

1/3

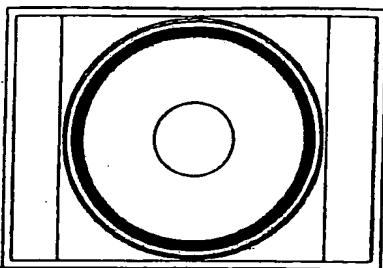


Fig. 1

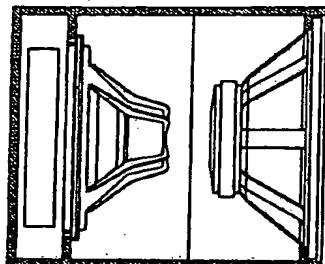


Fig. 1B

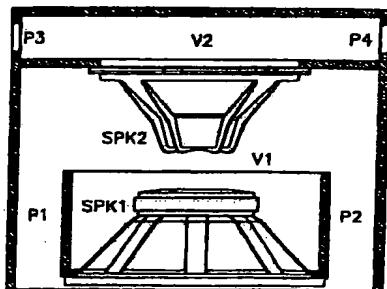


Fig. 1A


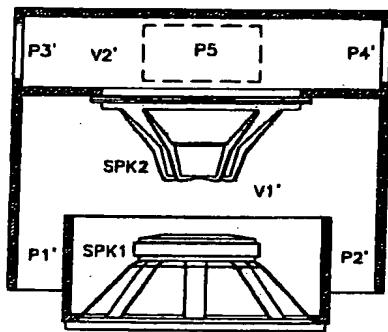


Fig. 2

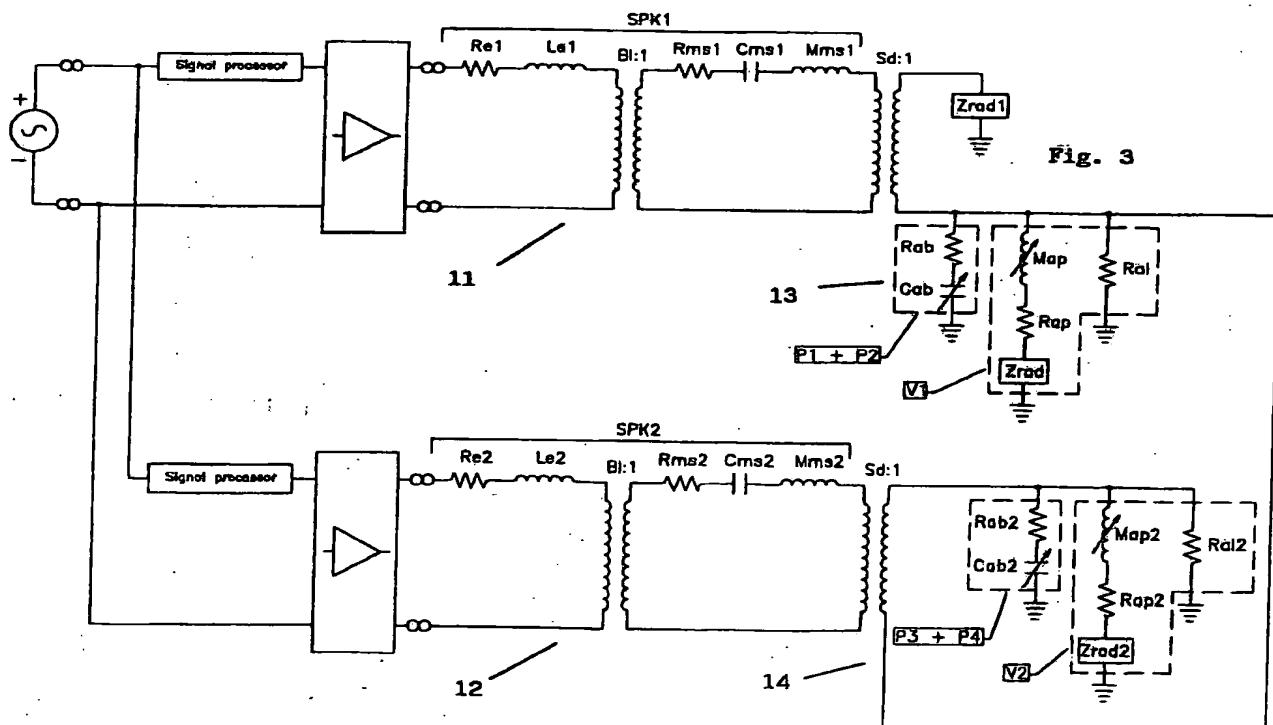

10/517300

2/3  
Ratio vs Angle

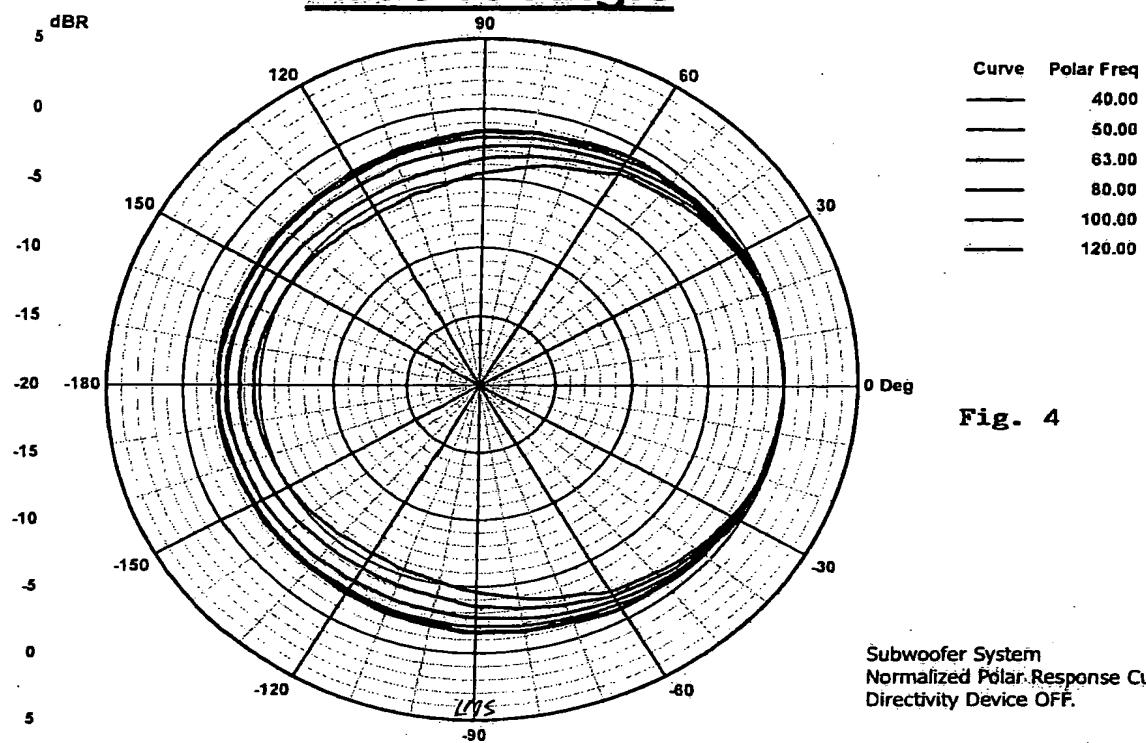


Fig. 4

Subwoofer System  
Normalized Polar Response Curve.  
Directivity Device OFF.

Ratio vs Angle

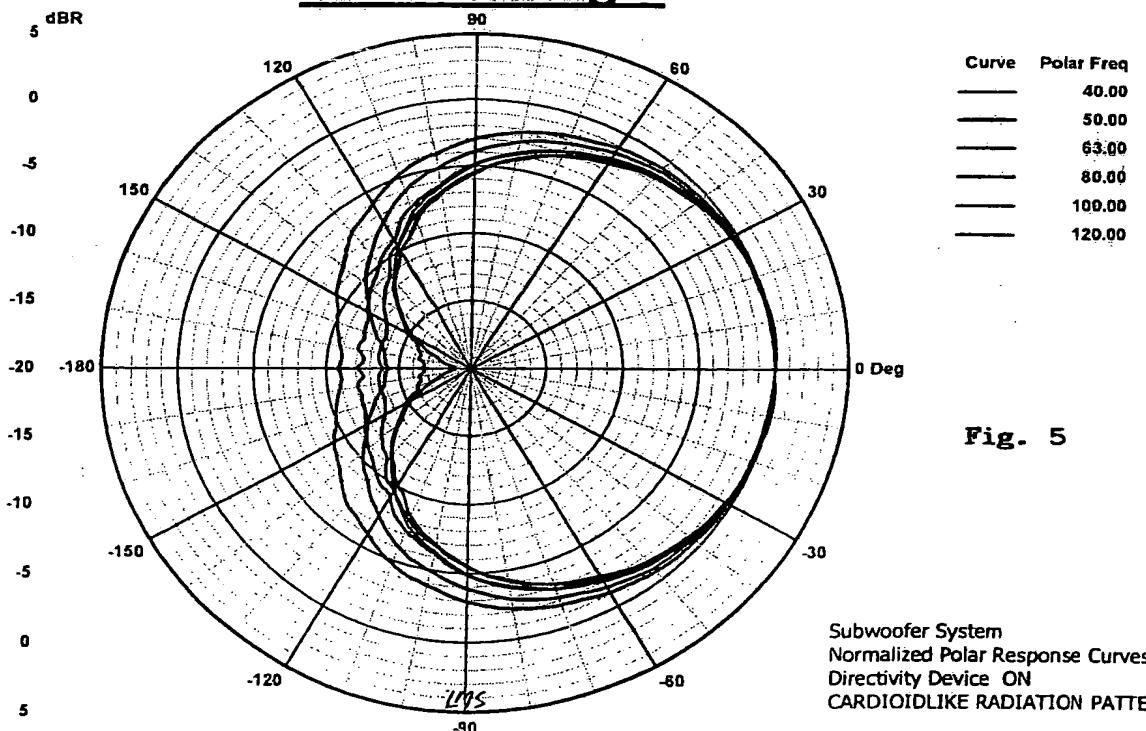


Fig. 5


Subwoofer System  
Normalized Polar Response Curves  
Directivity Device ON  
CARDIOIDLIKE RADIATION PATTERN

Best Available Copy

30/517300

3/3

### Ratio vs Angle

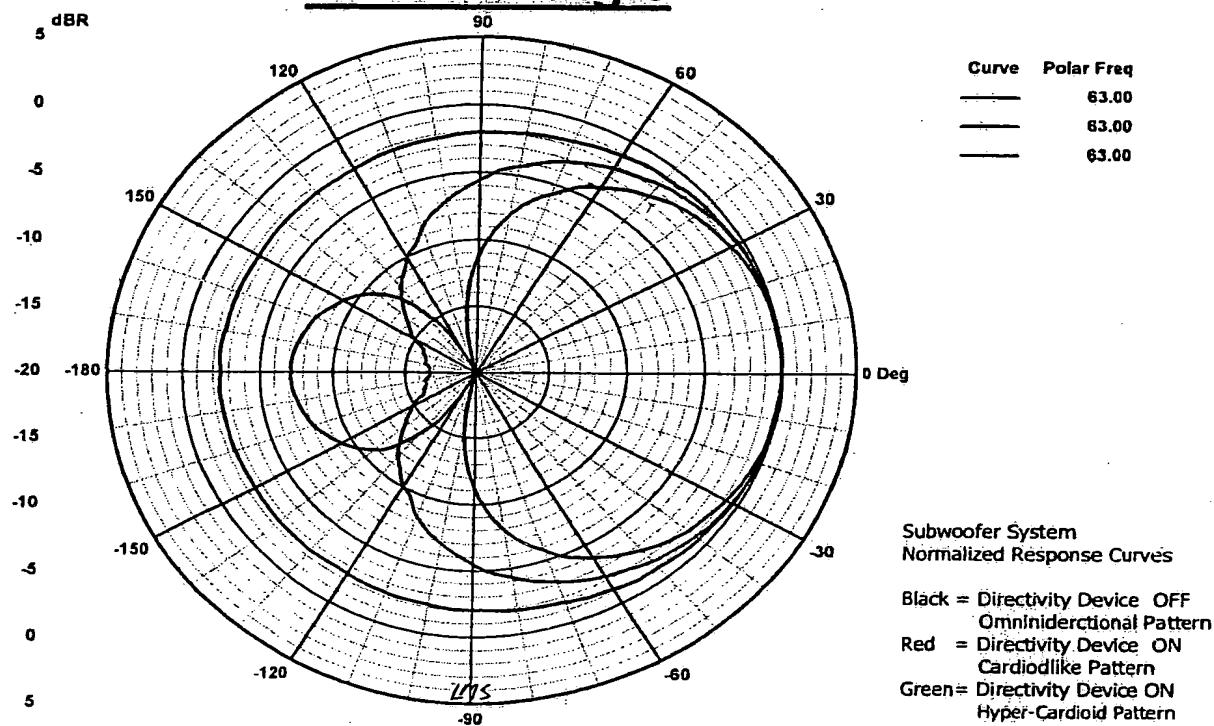

**Fig. 6**

**Best Available Copy**